


Fig. 1

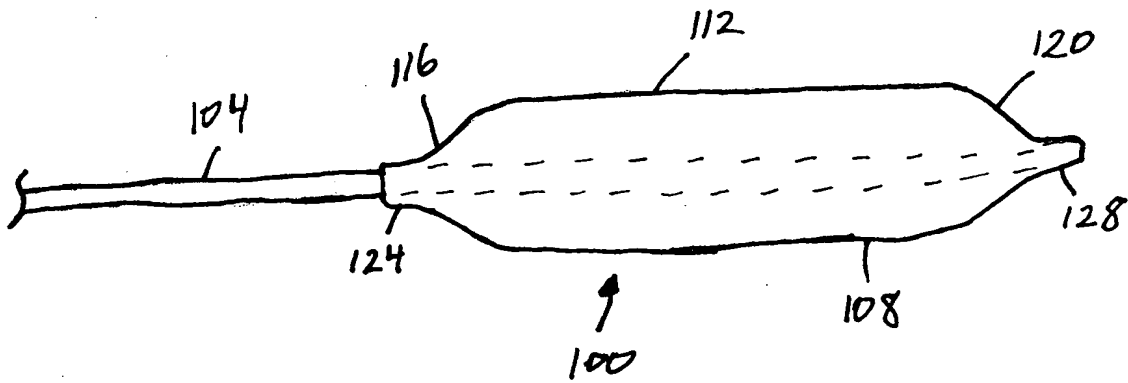

~~Fig. 1~~

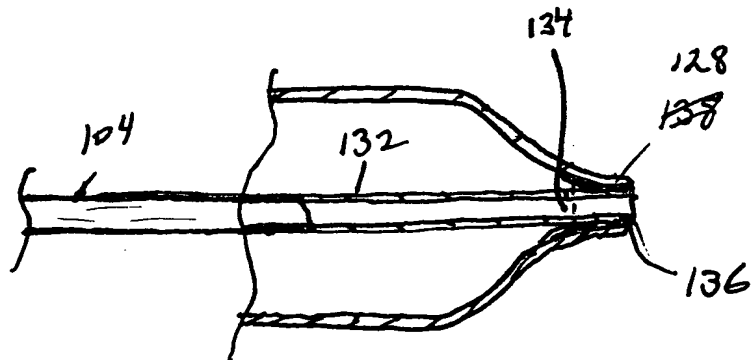


Fig. 2

03654987.050500

Fig. 3

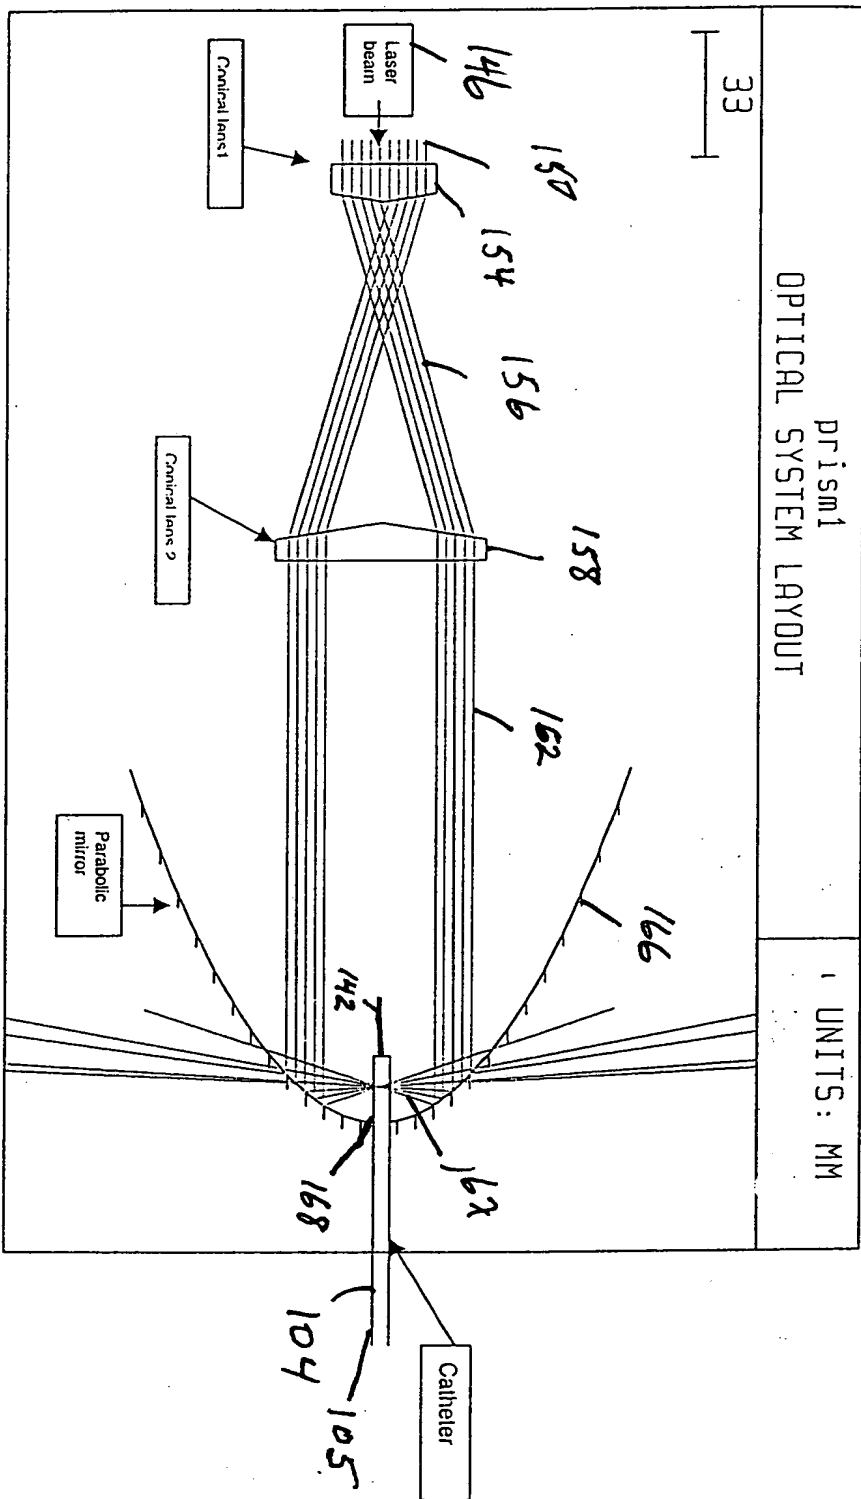


Figure 1: Design of the optical system

Figure 1: Design of the optical system

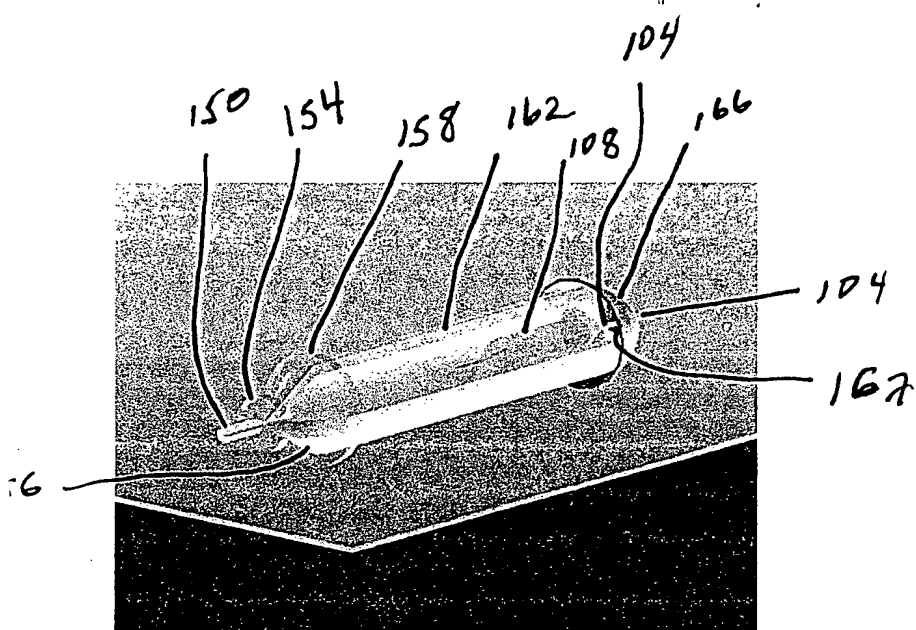


Fig. 4

035550 2364550

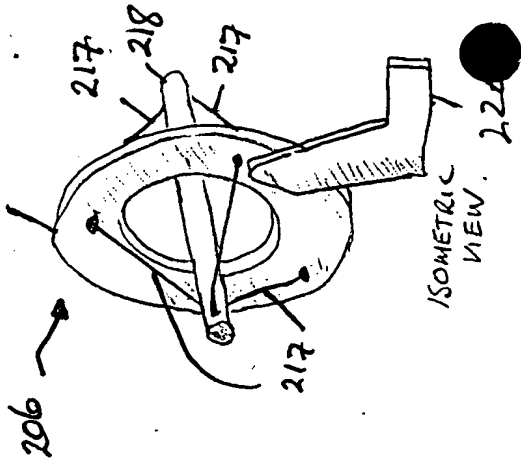


fig. 5b


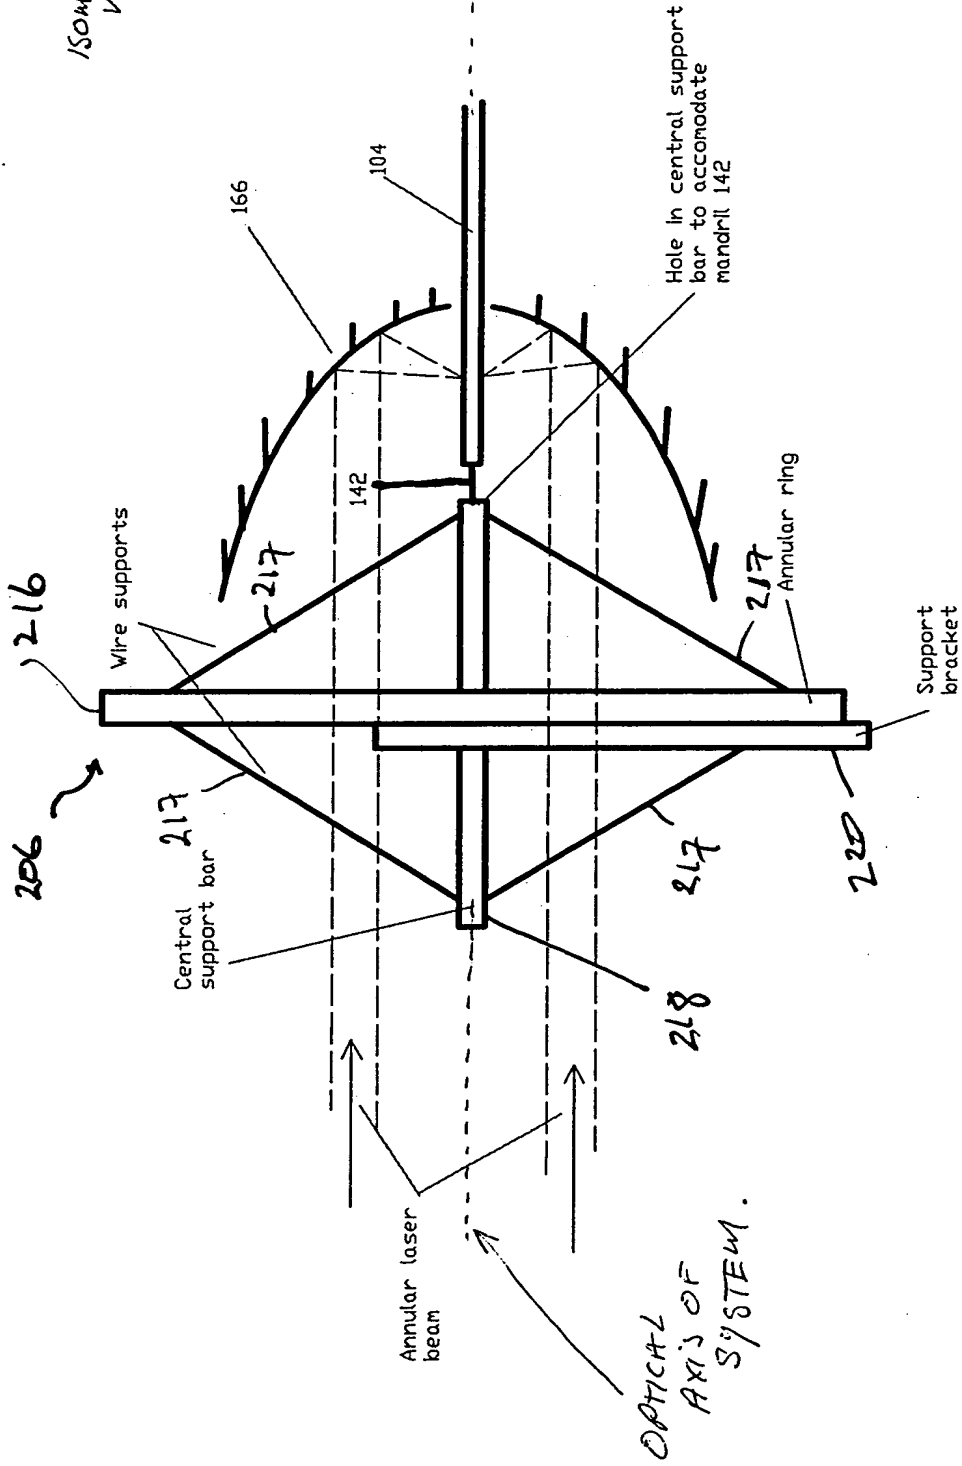


fig. 5a

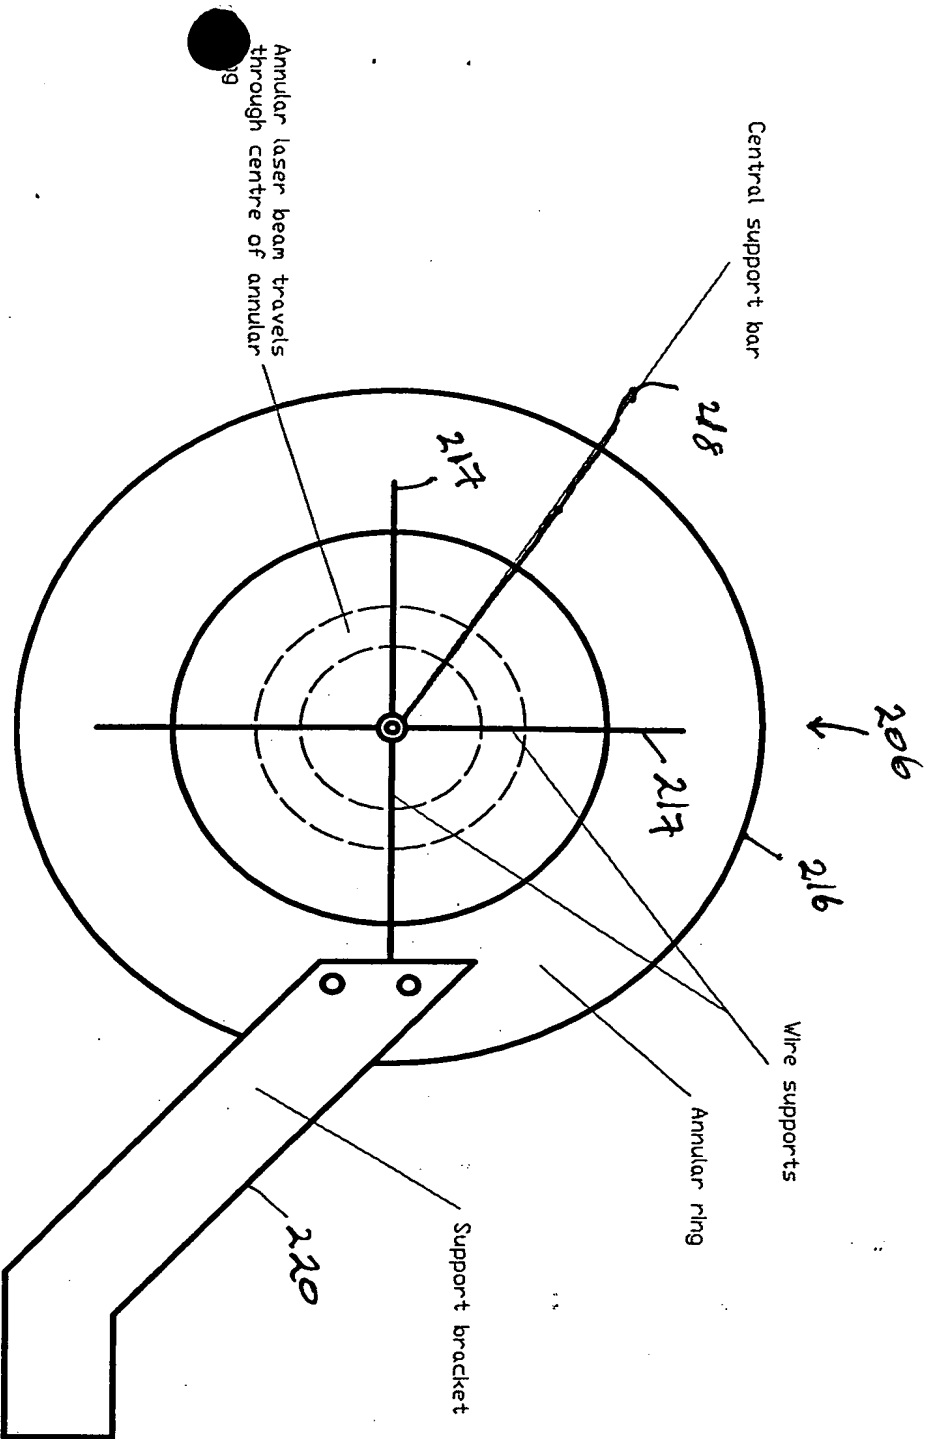

End view of the distal support fixture

03634937 090300

Fig. 5c

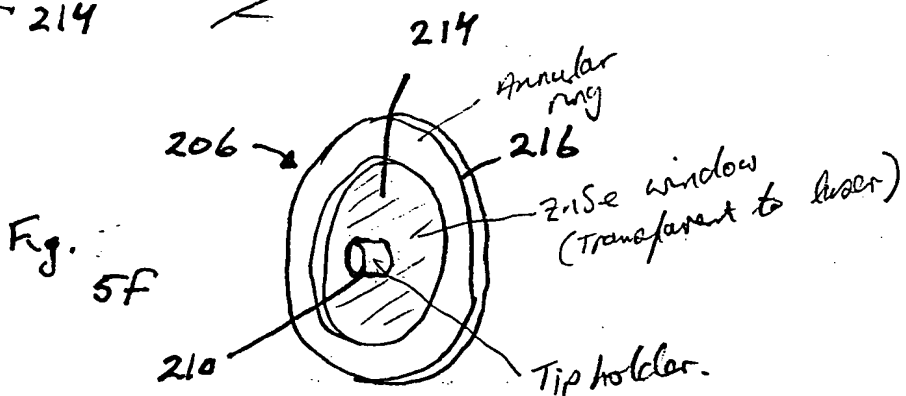
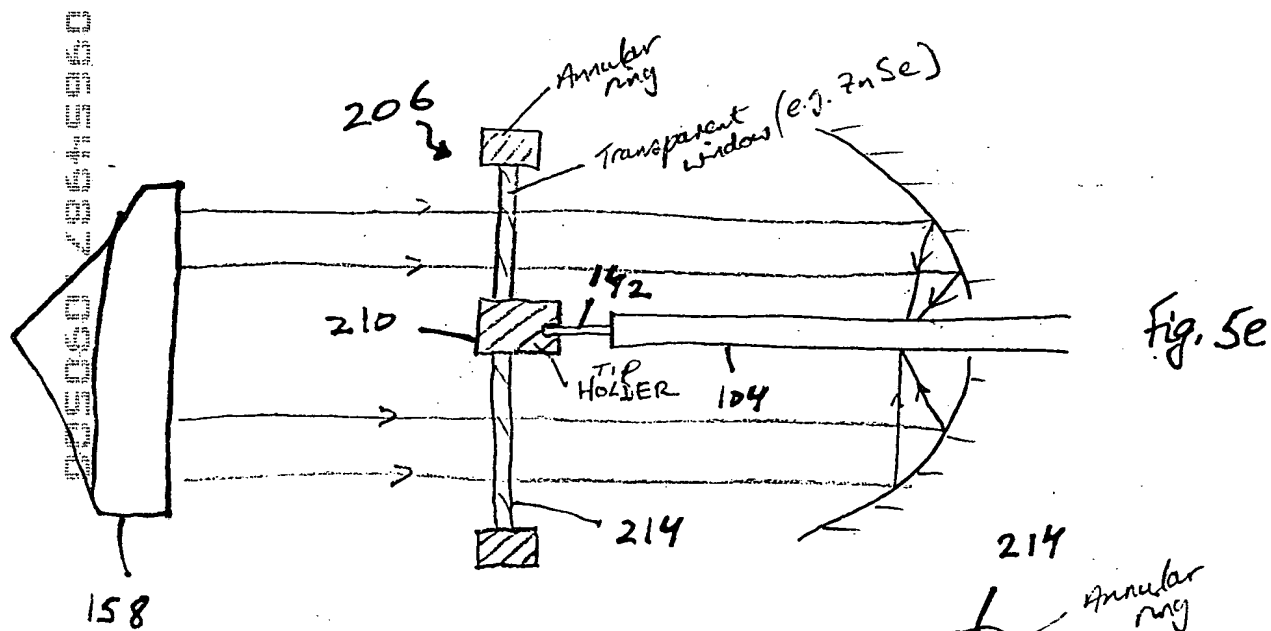
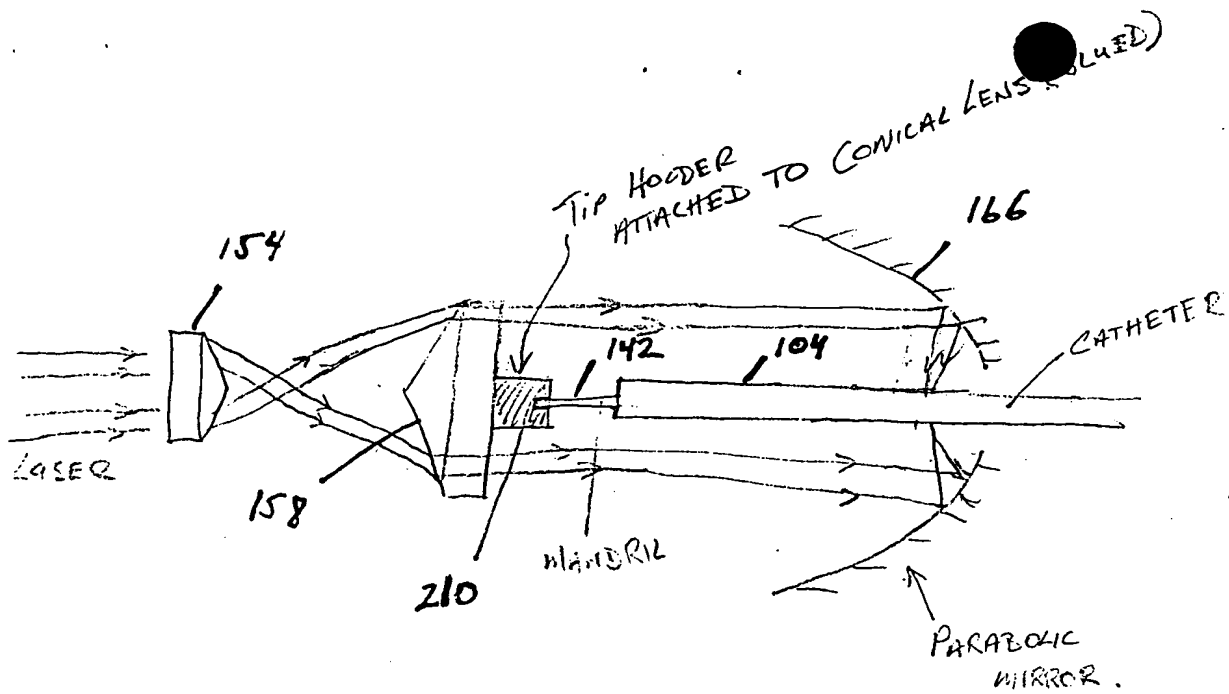
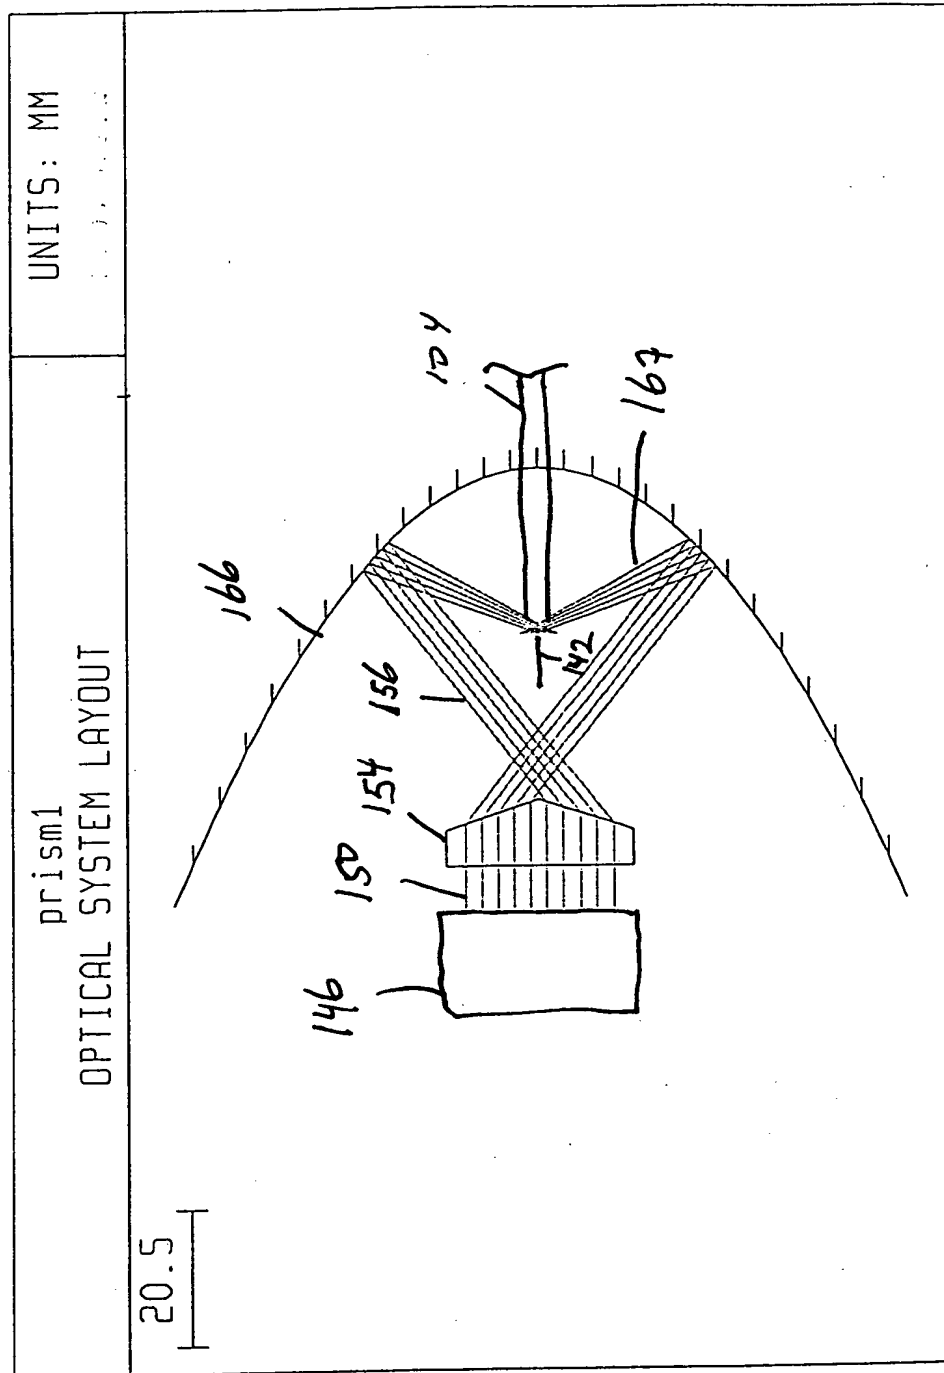


Fig. 7



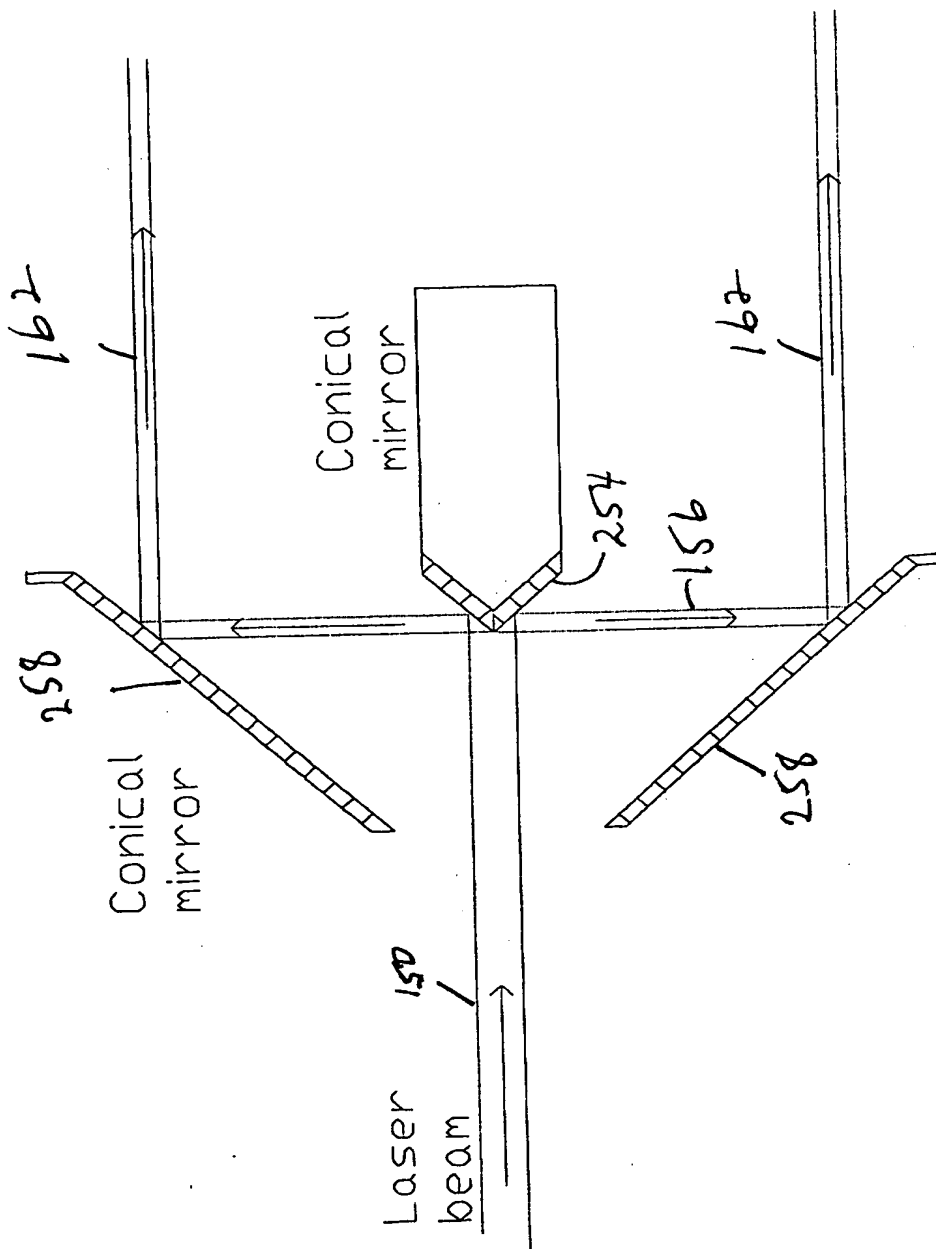


fig. 8

03654537 050500

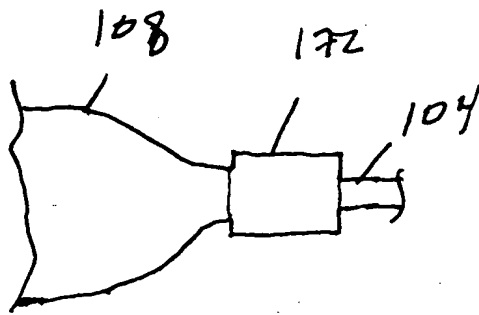


Fig. 9

Crosssection of beam (Radial)

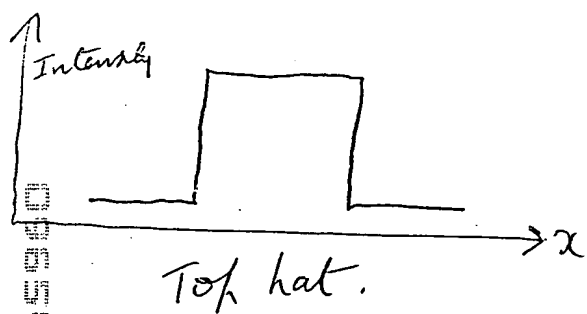


Fig. 10

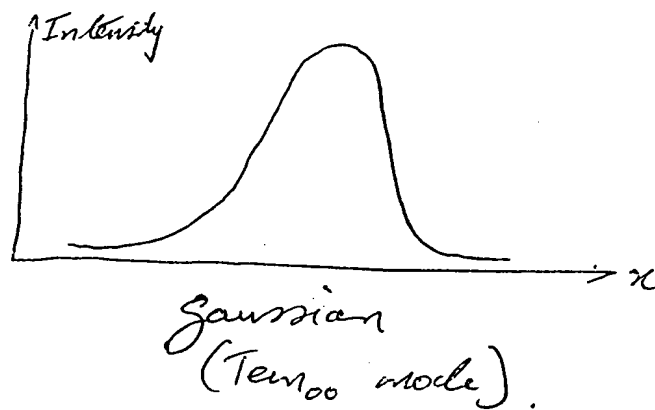


Fig. 11

Fig 12



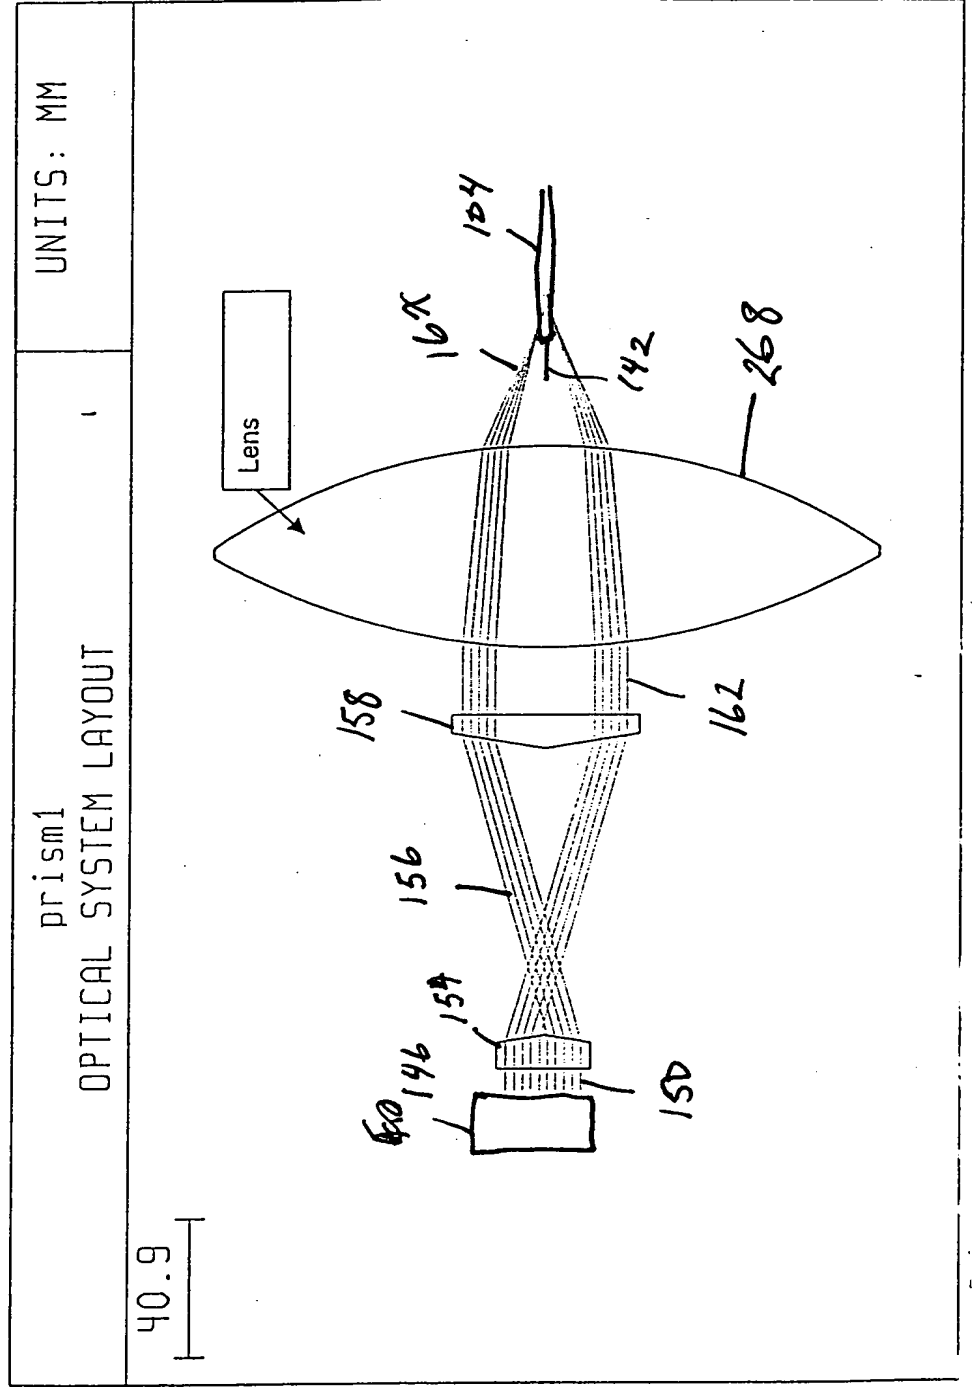


Fig. 13

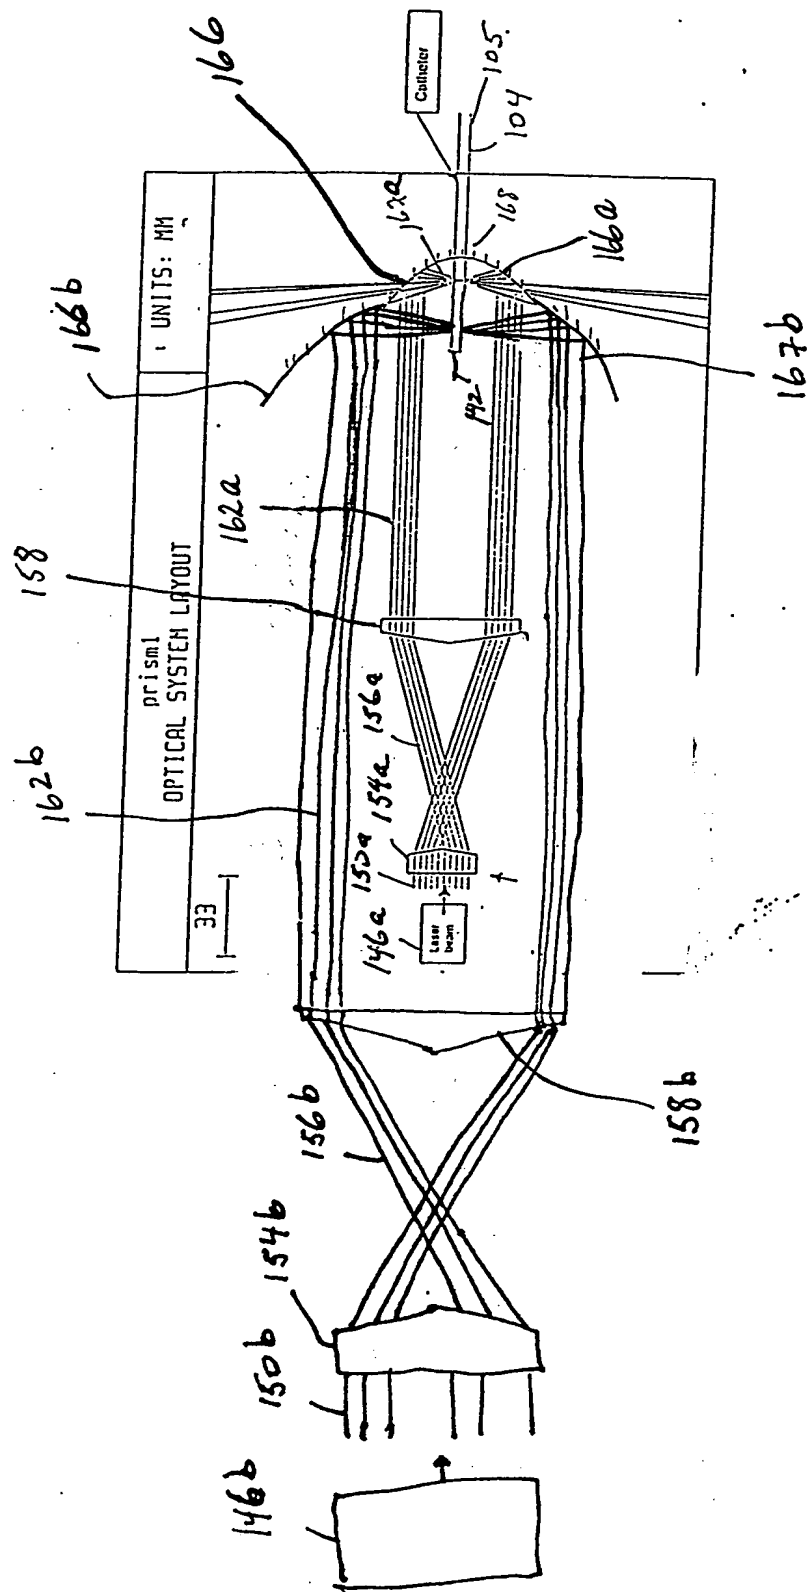

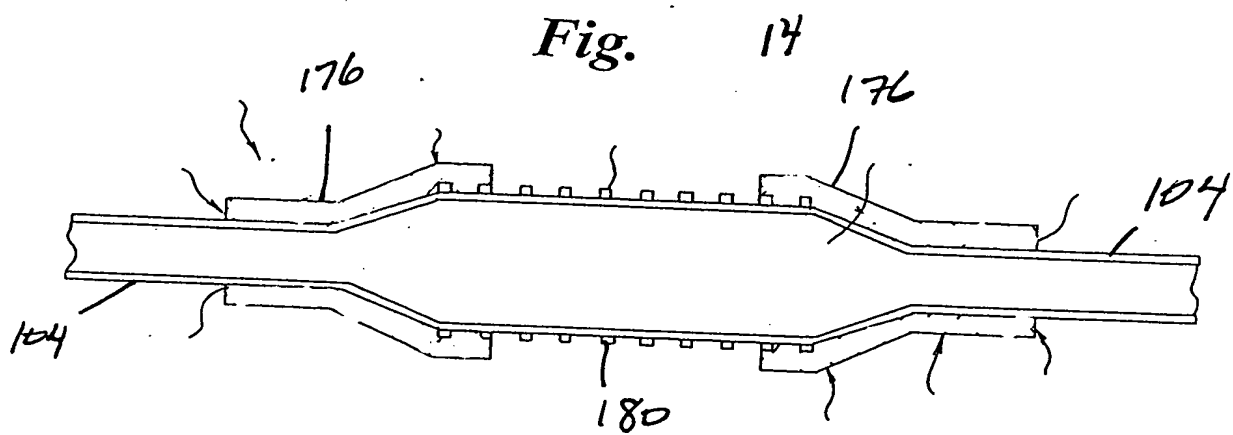

monorail catheters.

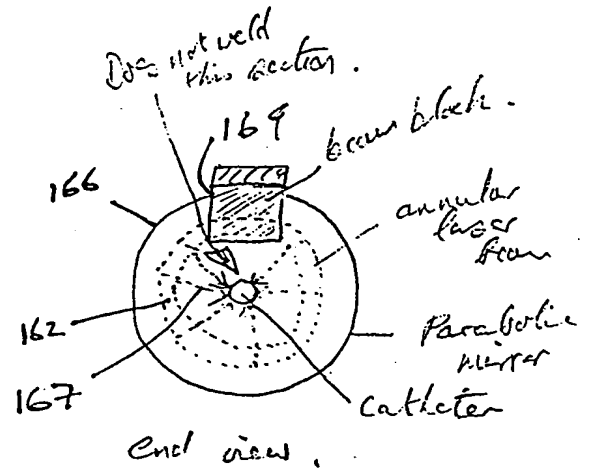
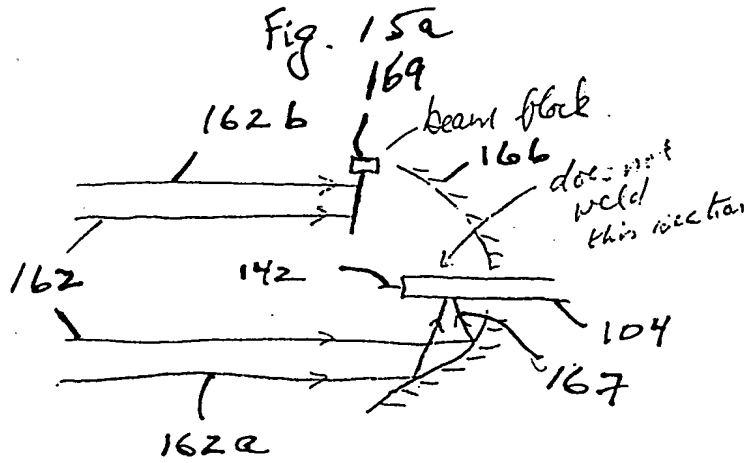


Fig. 15b

005060" 28645960